



OR Department Labeling Solutions

WARMED I.V. SOLUTION BAGS - JCAHO STANDARDS

JCAHO MEDICAL MANAGEMENT GUIDELINES

Under the MM20 General Storage Ruling for Stability of Meds - THE OPERATING ROOM IS REQUIRED to indicate the expiration DATE ON THE I.V. BAGS once the liquid has been warmed in the warmers. This requirement exists because the warming of the I.V. bags negates and shortens the manufacturers original warranty period for the sterility of their product.

Consequently, a new shortened expiration date needs to be *legibly* applied to the I.V. bag to satisfy JCAHO guidelines. Hand written dates, with a magic marker, can and have recently caused hospitals to be scrutinized by JCAHO for violating legibility requirements. Let **System One Medical** facilitate your labeling task to be 100% legible with JCAHO inspections requirements.

System One Medical offers

- Complete Customization for Label Tools
- Custom Label Pre-Prints
- FREE Technical Assistance to develop a cost effective and efficient label application with fast delivery



STOCK LABEL OPTIONS



Cat. No.: **L22-1018W**



Cat. No.: **L22-1018Y**



Cat. No.: **L22-1004**




Cat. No.: **L22-1023**



Cat. No.: **L22-1001**



Cat. No.: **L22-1017**

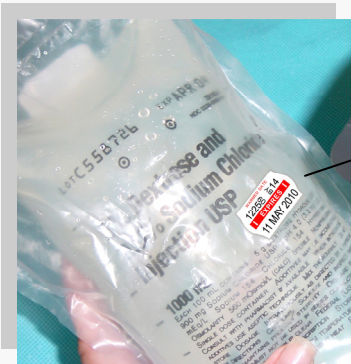

2 LINE TOOL
M20-0057

No Charge Label Tool !
With your first label purchase

M20 SERIES LABELING SYSTEM

item description	catalog number	label package
M20 - 2 LINE LABEL TOOL	M20-0057	24 roll /box - 1,250 labels /roll 1 ink roll FREE in each box
M20 INK ROLL SUPPLY	I22-0001	